


Attachment: ACT-541468 - AC-078A201

Predicted mean (95% CL) dose-response profile and LS means (95% CL) for change from baseline to Days 1&2 in WASO (min), Modified full analysis set

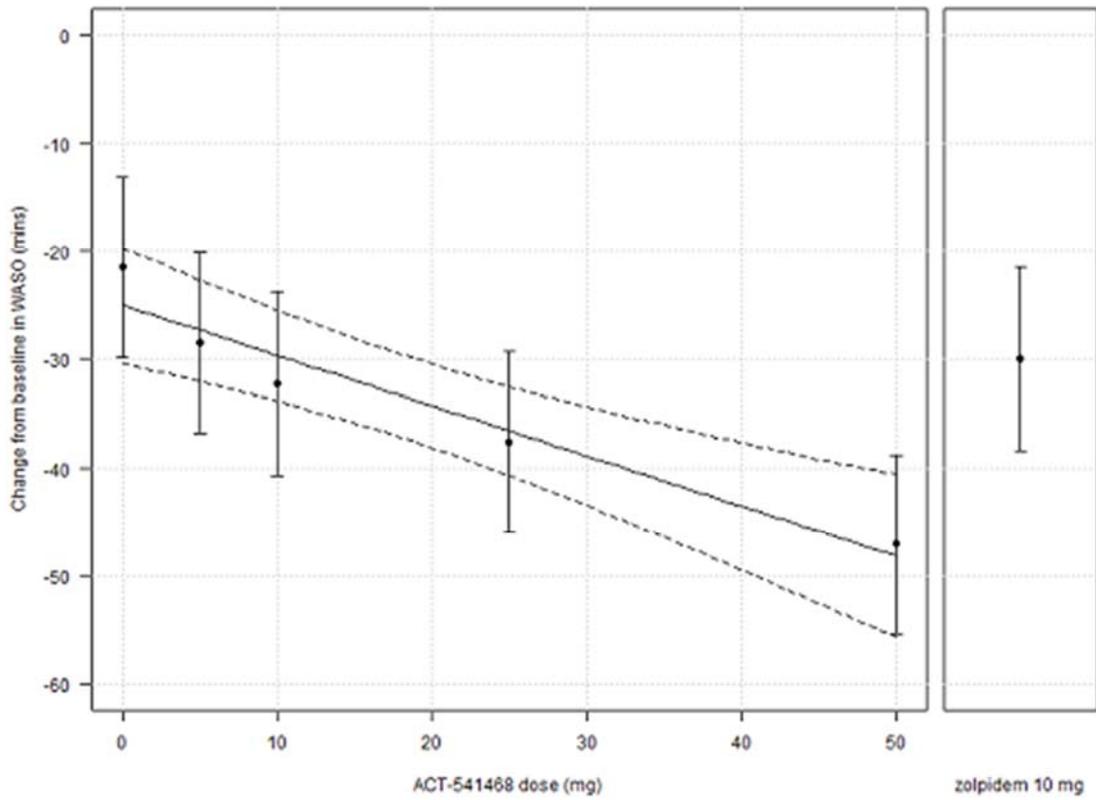

LS mean = least squares mean; CL = confidence limit